
Contact Information

Maintenance




To elevate seat section.

Lift seat until pelvic support drops into place.



To return seat section to flat position.

- A) Lift seat section slightly.
- B) Pivot pelvic support handle upward.
- C) Lower seat section.



Calling for Service

If service is required, contact Midmark directly. US 844.856.1230 / Canada 937.526.8585 Monday-Thursday 8:00 AM until 6:00 PM Friday 8:00 AM until 5:00 PM (ET)

English: Refer to midmark.com Deutsch: Siehe midmark.com

Français: Référez-vous à midmark.com

Español: Refiera a midmark.com

Dansk: Se midmark.com Suomi: Katso midmark.com

Italiano: fare riferimento a midmark.com

Svenska: Se midmark.com Norsk: Se midmark.com Nederlands: Zie midmark.com Polski: Patrz midmark.com Türkçe: midmark.com 'a bakın

Periodically inspect the following:

- · Power cord must be free of visible damage.
- Foot control cord must be free of visible damage.
- All fasteners must be present and secure.
- All mechanical functions should operate

Cleaning

Upholstery

Wash your upholstery weekly with a mild liquid soap and water mixture, rinse with clear water and dry completely to remove disinfection cleaner build-up.

Disinfect your upholstery with a solution of standard bleach and water mixed 1 in 10 (10%) or chlorine based cleaners (see current CDC Guideline for Disinfection and Sterilization in Healthcare Facilities). Follow this with a clear water rinse and thorough drying of material.

To minimize damage caused by disinfectant cleaner residue build-up, do not allow disinfectants to pool on the upholstery surface. Once the approved contact time has been obtained, remove and dry excess liquid remaining on the surface.

Detailed care and maintenance instructions are included with your product. This information is also available on <u>midmark.com</u> in the Technical library under the User Information tab for your product.


Painted Metal / Plastic Surfaces

Clean the painted metal and plastic surfaces weekly using a clean soft cloth and mild cleaner. Use of chlorine based disinfectant can cause damage to the hand control.


Midmark Corporation 60 Vista Drive Versailles, OH 45380 USA 1.800.643.6275 1.937.526.3662 midmark.com



Quick Reference Guide 627 (-011) Barrier-Free® Exam Chair

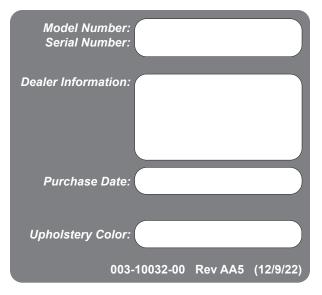

This guide outlines basic operation of the chair. The enclosed User Guide provides additional instructions on operation and care, as well as regulatory compliance information. If service is required, contact your authorized Midmark® dealer.




Note

The chair automatically stops at its maximum and minimum height.

To move the chair up or down.

Press and hold the appropriate button.

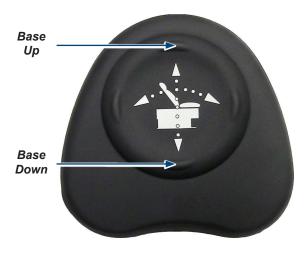


Note


The back section automatically stops at the top and bottom of its travel.

To position the back section.Press and hold the appropriate button.



<u>Max.</u> 94 ± 1.3 cm (37 ± 0.5 in.)



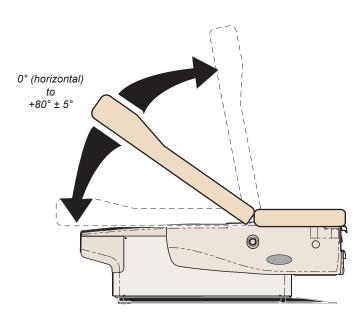

MA10293i