Tray (9" x 13") Installation Guide

Applies to Models:
153634-001 (Field Installation)

Special Tools:
None

Language of origin: English

Step 4: Check operation. If necessary, adjust drag using the screws at two pivot points.

Note: Prior to reinstall, place a small bead of silicone on inside of cap to secure it.

Note
If necessary, prior to reinstall, place a small bead of silicone on inside of cap to secure it.

Step 2: The mounting plug is held in place with silicone. Tap it out from bottom side.

Note
Tray assembly can be mounted to from the Doctor's Instrument Head to extend outward to the left or the right.
Determine desired direction before mounting.

Note
Maximum shelf load limitations is 5 lbs. (2.3 kg).
Check level of delivery unit and/or arm. Refer to Leveling of Delivery Unit or L/R Deliery Arm Leveling in Service Manual.

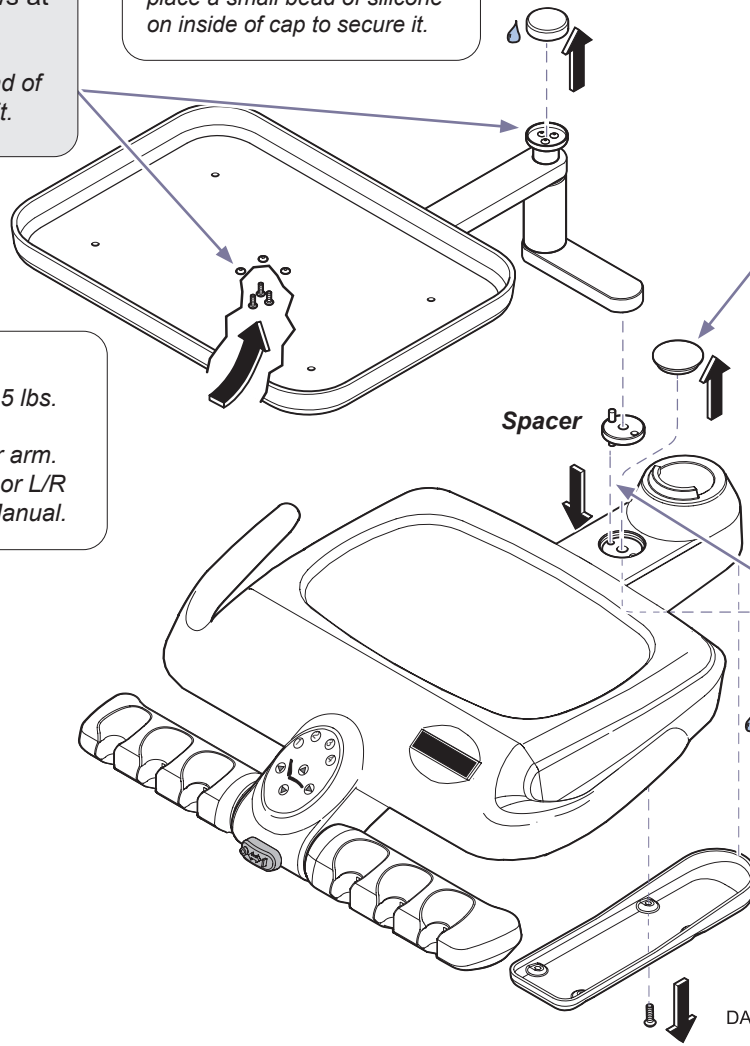

Step 3: Position tray assembly so dowel pin in spacer is located in the correct hole in the base for desired left or right mounting. Secure with flat washer and 1/4"-20 x 3/4" bolt.

Note: Place a small drop of non-permanent threadlock on screw.

Step 1: Remove the bottom cover.