

Warranty

SCOPE OF WARRANTY

Midmark Corporation ("Midmark") warrants to the original purchaser its Exam Room Casework, Veterinary products and components (except for components not warranted under "Exclusions") manufactured by Midmark to be free from defects in material and workmanship under normal interior use and service. Midmark's obligation under this warranty is limited to the repair or replacement, at Midmark's option, of the parts or the products the defects of which are reported to Midmark within the applicable warranty period and which, upon examination by Midmark, prove to be defective.

APPLICABLE WARRANTY PERIOD

The applicable warranty period, measured from the date of delivery to the original user, shall be as follows: • **The VetPro® 5000 unit is warranted against defect in material and workmanship for a period of two years from the time of delivery.**

DENTAL PRODUCTS are warranted against defect in material and workmanship for the period indicated below from the time of delivery: a) 2 years for all products and components (except for the periods in b through d).

b) "KINK-VALVE" module carries a 10 year warranty.

c) Accessories not manufactured by Midmark are excluded (i.e. Fiber optic systems, Scalers, Handpieces, etc.). d) Replacement parts and accessories carry a 90 day warranty.

EXCLUSIONS

This warranty does not cover and Midmark shall not be liable for the following; (1) repairs and replacements required because of misuse, abuse, negligence, alteration, accident, freight damage, or tampering; (2) changes in color caused by natural or artificial light; (3) products which are not installed, used, and properly cleaned as required in the Midmark written "Installation" and or "Installation/Operation" Manual applicable for this product; (4) products considered to be of a consumable nature such as light bulbs and surge suppression product; (5) accessories or parts not manufactured by Midmark; (Any warranties on these items are extended directly by the manufacturer of these items to the original purchaser.

Information on these manufacturers' warranties will be enclosed with the applicable products. Also, Midmark will furnish copies of any of the warranties extended by any such manufacturers upon request.) (6) specially manufactured products; (7) damage caused by animals; (8) charges by anyone (including Midmark's authorized dealers) for adjustments, repairs, replacement parts, installation, or other work performed upon or in connection with such products which is not expressly authorized in writing in advance by Midmark.

EXCLUSIVE REMEDY

Midmark's only obligation under this warranty is the repair or replacement of defective parts. Midmark shall not be liable for any direct, special, indirect, incidental, exemplary or consequential damages or delay including, but not limited to, damages for loss of profits or loss of use.

Warranty Continued...

SCOPE OF WARRANTY

Midmark Corporation ("Midmark") warrants to the original purchaser its Exam Room Casework, Veterinary products and components (except for components not warranted under "Exclusions") manufactured by Midmark to be free from defects in material and workman


NO AUTHORIZATION

No person or firm is authorized to create for Midmark any other obligation or liability in connection with the products.

THIS WARRANTY IS MIDMARK'S ONLY WARRANTY AND IS IN LIEU OF ALL OTHER WARRANTIES, EXPRESSED OR IMPLIED. MIDMARK MAKES NO IMPLIED WARRANTIES OF ANY KIND INCLUDING ANY WARRANTIES OF MERCHANTABILITY OR FITNESS FOR ANY PARTICULAR PURPOSE. THIS WARRANTY IS LIMITED TO THE REPAIR OR REPLACEMENT OF DEFECTIVE PARTS.

To activate warranty:

Insert CD, then select Product Registration from the menu.

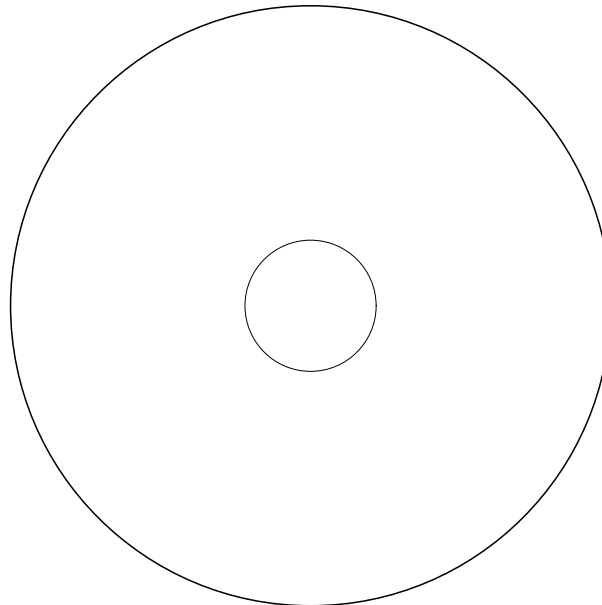

Annual Maintenance Kits



Bronze Muffler

Order#: 002-1143-00



Filter for Plastic Muffler

Order#: 002-1149-00

Calling for Service

If service is required, contact your Midmark dealer.

To contact Midmark directly:

1-800-Midmark (1-800-643-6275)

8:00am until 5:00 pm Monday through Friday (EST)

Midmark Corporation
60 Vista Drive
Versailles, OH 45380-0286
Phone: 937-526-3662
Fax: 937-526-5542
www.midmark.com



Because we care.



Operating and Care Guide VetPro® Solo

Model Number:
Serial Number:

Dealer Information:

Purchase Date:


Upholstery Color:

003-2006-00 Rev B

The operation of the VetPro® Solo Compress System is restricted to use by veterinary professionals.

This guide outlines basic care and maintenance of the VetPro® Dental Systems. The enclosed CD provides additional instructions on operation and care. If service is required, contact your authorized Midmark dealer.

Important Information

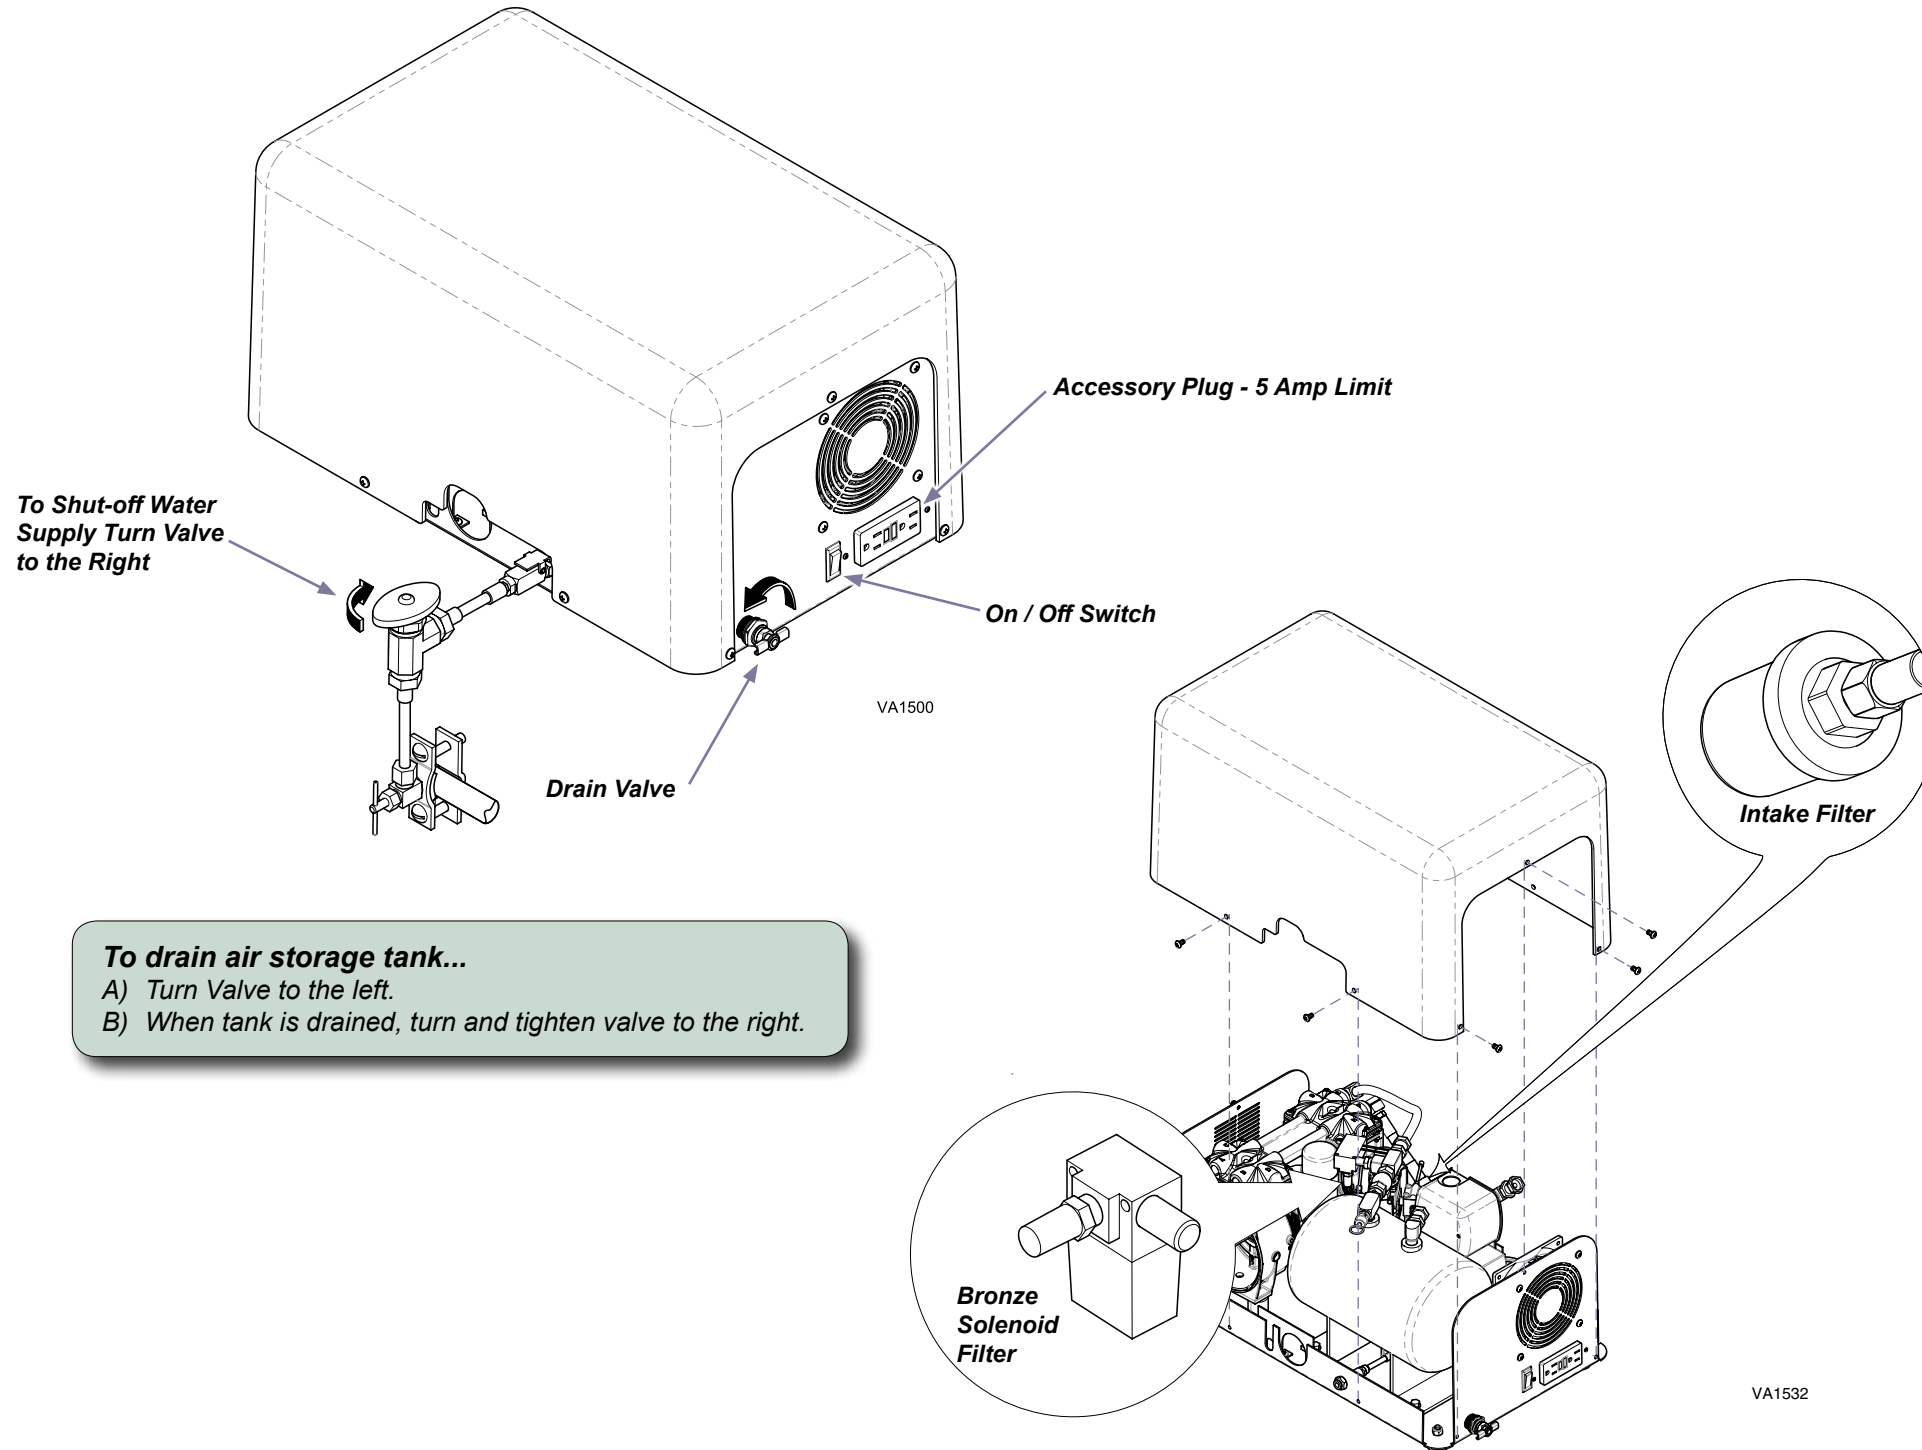

Daily

A. Drain Condensation from Air Tank.

Monthly

A. Clean System

- Wipe with a clean cloth to remove dust and debris.

Annually

A. Replace Air Intake Filter

- Contact Midmark Authorized Service Technician.

B. Replace Bronze Filter

- Contact Midmark Authorized Service Technician.