



Scale / USB PC Board Kits [002-1512-00 / 002-1514-00 / 002-1515-00 / 002-1516-00]

Components:
PC Board......1


Special Tools:

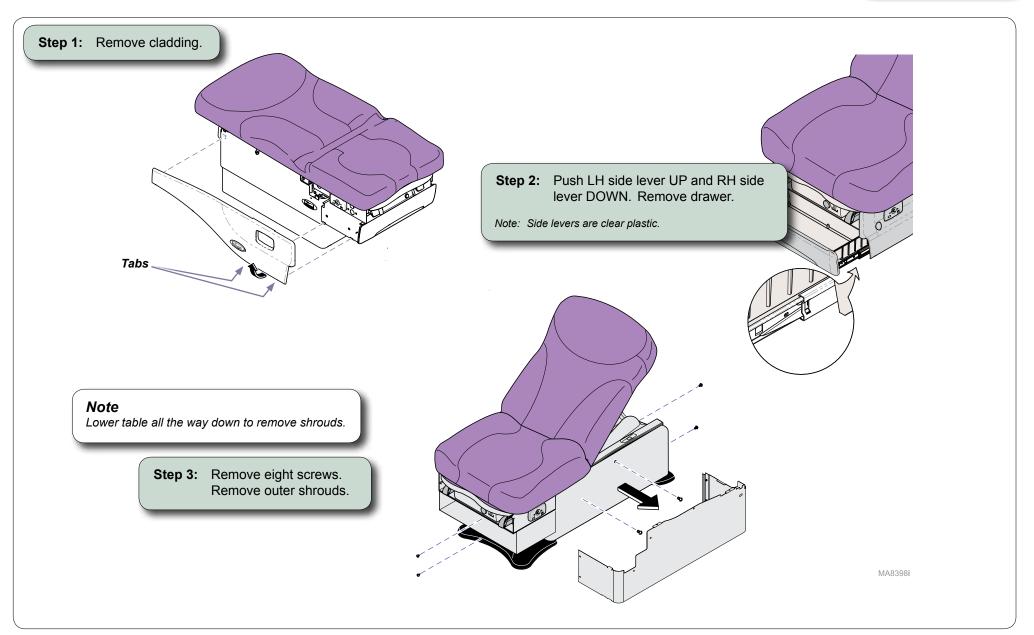


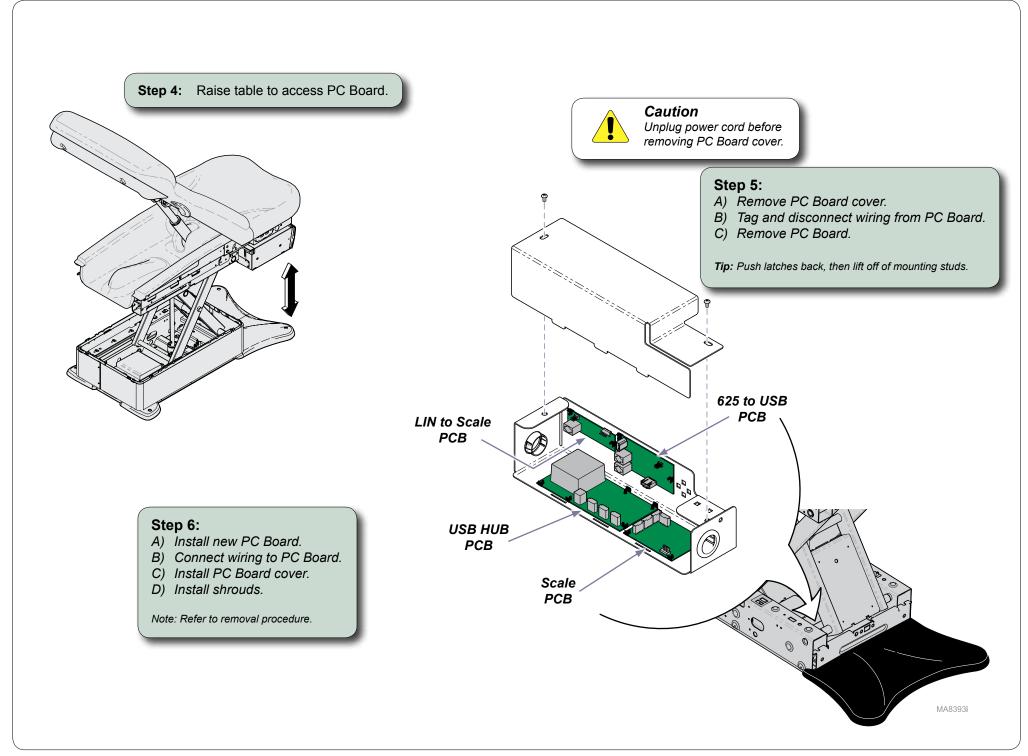

Step 7:

- A) Insert tab at head-end of cladding into top shroud.
- B) Slide cladding over upperwrap.
- C) Pull bottom of cladding out, then push down on the top to engage the long tab onto top edge of upperwrap.
- D) Push bottom of cladding in, until two bottom tabs snap into place.

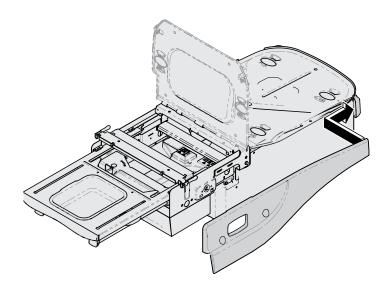

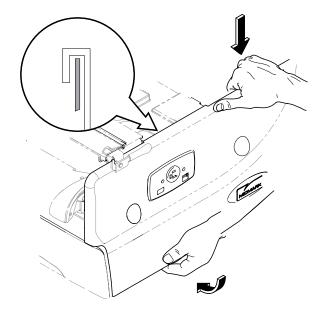

Step 8: Perform Scale Calibration Procedure.

Note: For 002-1512-00 Scale PCB Only.

Scale Calibration Procedure

Step 1:

- A) Remove any load from the patient surface.
- B) Press and hold the Weight and Plus buttons until "Pause" is displayed for at least one second, then release buttons.

Step 2:

- A) When "CLrAL" is displayed, firmly press and release the plus button.
- B) After count down, "Ad50" will be displayed.







Step 3:

- A) Place fifty pound calibrated weight on patient surface.
- B) Firmly press and release the plus button. Note: After count down "donE" will be displayed.



- A) Wait until display clears, then firmly press and release the weight button. Note: "50 lbs" should be displayed.
- B) Remove calibrated weight.



